



# NC State Standard

Cytometer:	LSRII	User:	Sarah
Cytometer Name:	LSRII	Institution:	
Serial Number:	1	Software:	BD FACSDiva 6.1.3
Input Device:	Manual	Date:	5/19/2014 10:46:58 AM
Window Extension:	10.00		


Blue Laser  
(488nm)  
FSC

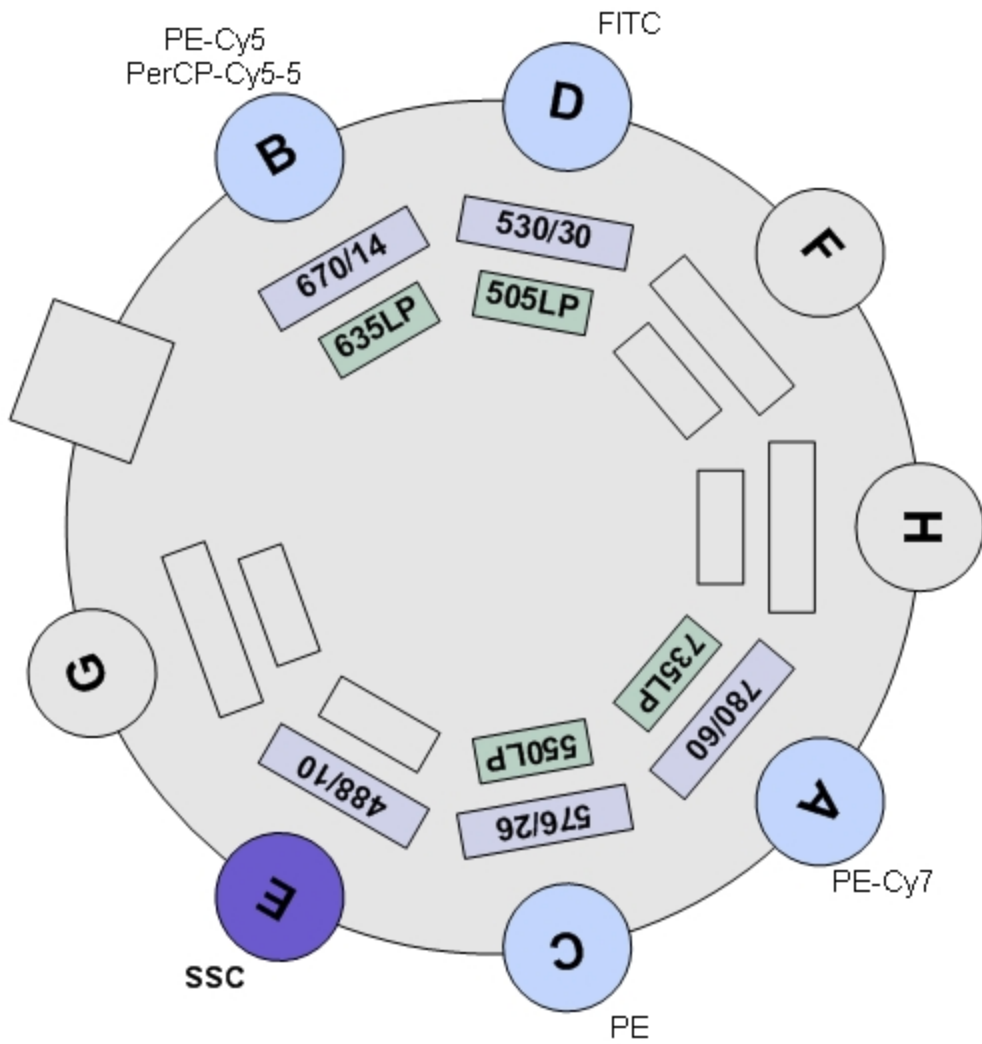


Violet Laser  
(405nm)

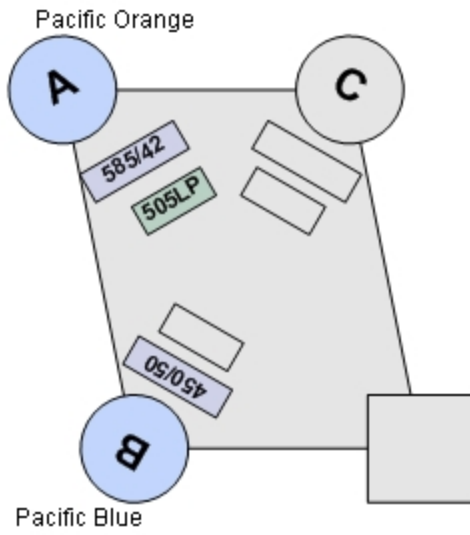

Red Laser  
(633nm)

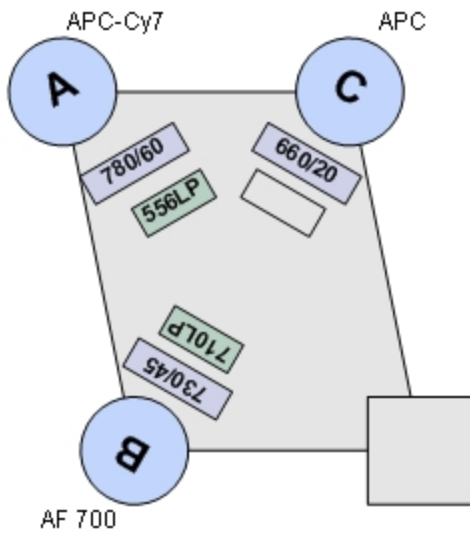

place holder Laser  
FSC

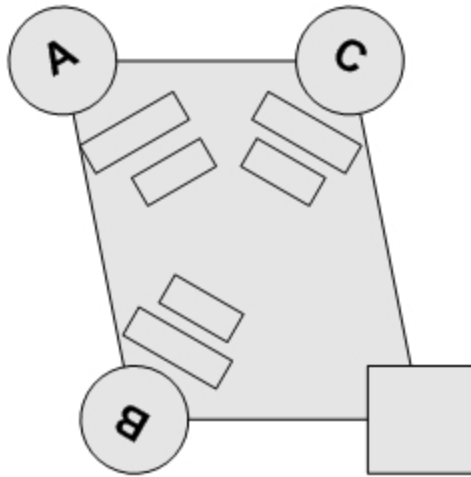

Comments: \_\_\_\_\_